



TEST REPORT TUCHENG

ORIGINAL

Date of Issue: Nov. 17, 2020 Date of Receipt and Test Start: Oct. 28, 2020


Report No.: TFF9J681 Quantity: 1PC Page Order/Pages: (P1/2) Ref. No.: NIL

Report Title: ATARAXIS MEDICAL SUPPLY CO., LTD. (U3494) Item: Mask

Address: 2F., No. 14, Ln. 122, Sec. 2, Xiwan Rd., Xizhi Dist., New Taipei City 221, Taiwan (R.O.C.)

Test Items		Test Results	Test Methods
Particulate Filtration Efficiency(%) (0.1 μm PSL)	1	99.37	CNS 14774 T5017-2018
	2	99.39	9.3(a)
	3	99.38	ASTM F2299-2017
	4	99.38	Flow rate:28.1
	5	99.38	(Liter/min)
	Ave.	99.38	

Note: Sample description is given by the client: ATARAXIS 3D DISPOSABLE FACE MASK

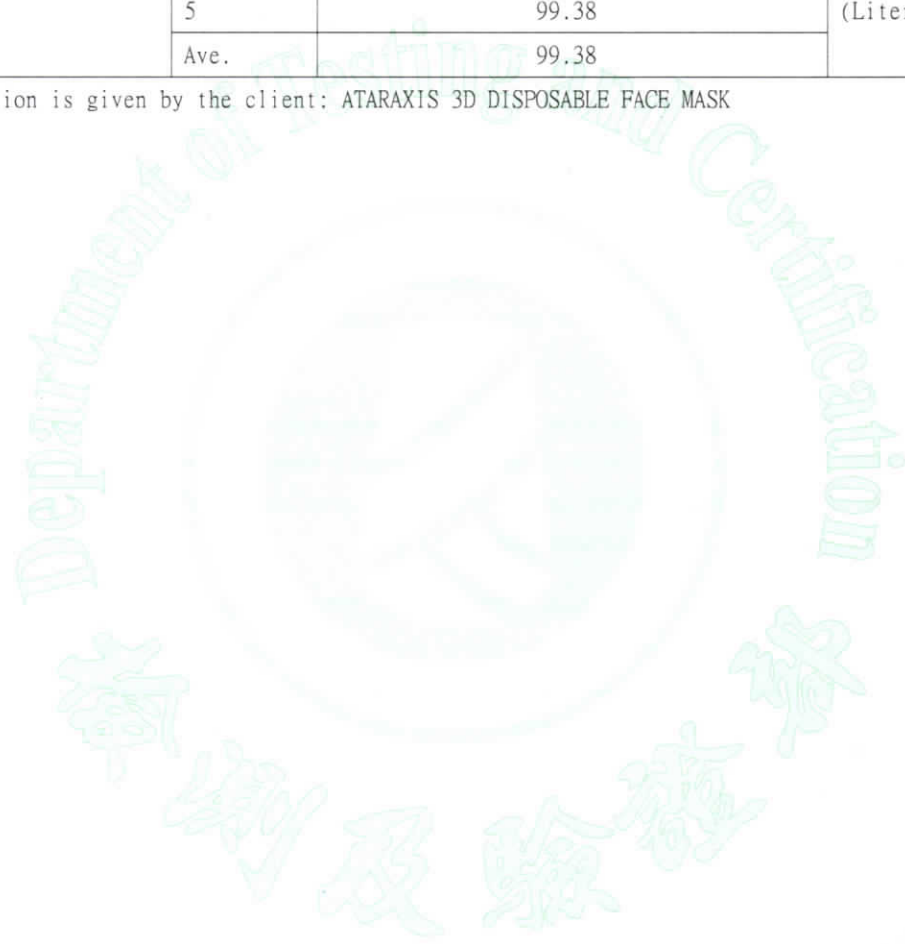

- Note: 1.This report is only responsible for the submitted sample(s), which will be kept for one month period.
- 2.This report cannot be reproduced in any way, except in full context, without the prior approval in writing of this Department of Testing and Certification.
- 3.The test report should not be used for public advertisement and commercial promotion.

Authorized by president of Jui-hung kao
Taiwan Textile Research Institute

Director,
Department of Testing and Certification

Department of Testing and Certification, Taiwan Textile Research Institute
No.6, Chengtian Rd., Tucheng Dist., New Taipei City 23674, Taiwan (R.O.C.)
Tel : +886-2-22670321 ext. 7107, 7110
Fax : +886-2-22675108 , +886-2-22689839

TEST REPORT TUCHENG

ORIGINAL

Date of Issue: Nov. 17, 2020 Date of Receipt and Test Start: Oct. 28, 2020

Report No.: TFF9J681 Quantity: 1PC Page Order/Pages: (P2/2) Ref. No.: NIL

Report Title: ATARAXIS MEDICAL SUPPLY CO., LTD. (U3494) Item: Mask

Address: 2F., No. 14, Ln. 122, Sec. 2, Xiwán Rd., Xizhi Dist., New Taipei City 221, Taiwan (R.O.C.)



- Note: 1.This report is only responsible for the submitted sample(s), which will be kept for one month period.
- 2.This report cannot be reproduced in any way, except in full context, without the prior approval in writing of this Department of Testing and Certification.
- 3.The test report should not be used for public advertisement and commercial promotion.

Authorized by president of Jui-hung Kuo
Taiwan Textile Research Institute

**Director,
Department of Testing and
Certification**

Department of Testing and Certification, Taiwan Textile Research Institute
No.6, Chengtian Rd., Tucheng Dist., New Taipei City 23674, Taiwan (R.O.C.)

Tel : +886-2-22670321 ext. 7107, 7110

Fax : +886-2-22675108 , +886-2-22689839