



TEST REPORT TUCHENG

Date of Issue: Oct.08,2021 Date of Receipt and Test Start: Sep.17,2021

Report No.: TFG01311 Quantity: IPC Page Order/Pages: (P1/4) Ref. No.: NIL

Report Title: ATARAXIS MEDICAL SUPPLY CO., LTD.(U3494) Item: Mask


Address: 2F., No. 14, Ln. 122, Sec. 2, Xiwan Rd., Xizhi Dist., New Taipei City 221, Taiwan (R.O.C.)

Test Items	Test Results	Test Methods
Air Exchange Pressure (Pa/cm ²)	1	31.1
	2	27.7
	3	29.9
	4	29.7
	5	28.5
		EN 14683:2019 Annex C Flow rate: 8 (Liter/min)

This test report is for reference only and should not be used as a formal document.

Note: Air Exchange Pressure testing area: 4.9 cm².

Note: Sample description is given by the client: ATARAXIS MEDICAL FACE MASK TYPE: II

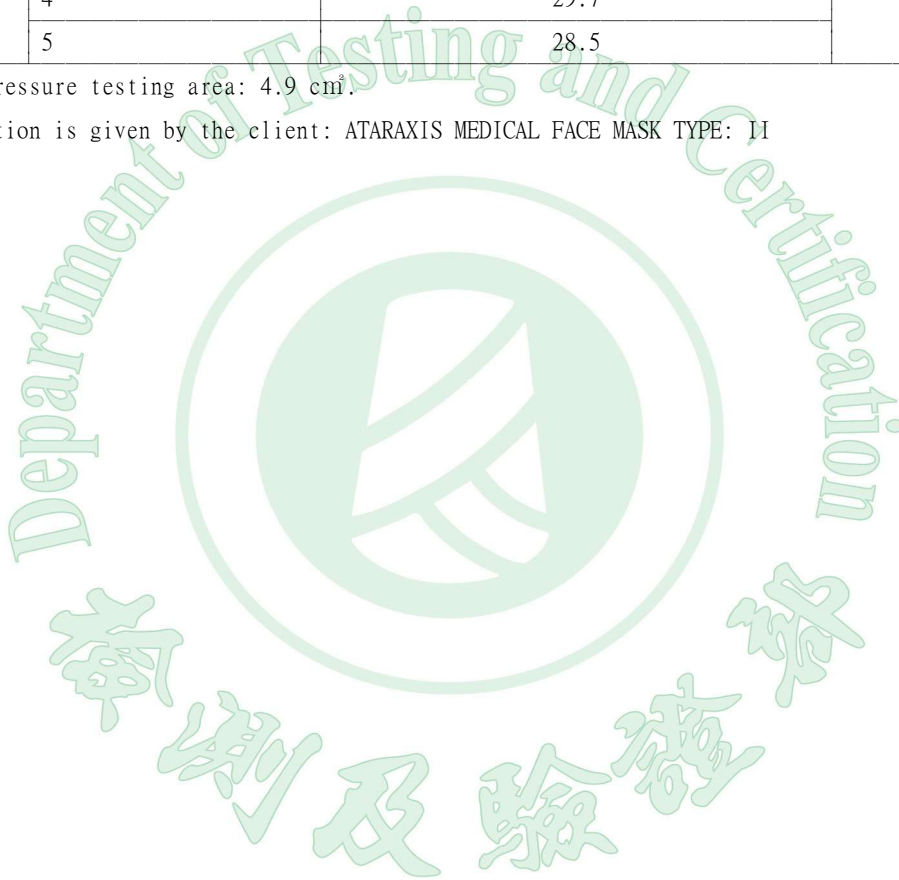

- Note: 1.This report is only responsible for the submitted sample(s), which will be kept for one month period.
2.This report cannot be reproduced in any way, except in full context, without the prior approval in writing of this Department of Testing and Certification.
3.The test report should not be used for public advertisement and commercial promotion.

Authorized by president of Jui-hung kao
Taiwan Textile Research Institute
Director,
Department of Testing and Certification

Department of Testing and Certification, Taiwan Textile Research Institute
No.6, Chengtian Rd., Tucheng Dist., New Taipei City 23674, Taiwan (R.O.C.)
Tel : +886-2-22670321 ext. 7107, 7110
Fax : +886-2-22675108 , +886-2-22689839



TEST REPORT TUCHENG

Date of Issue: Oct.08,2021 Date of Receipt and Test Start: Sep.17,2021

Report No.: TFG01311 Quantity: IPC Page Order/Pages: (P2/4) Ref. No.: NIL

Report Title: ATARAXIS MEDICAL SUPPLY CO., LTD.(U3494) Item: Mask

Address: 2F., No. 14, Ln. 122, Sec. 2, Xiwán Rd., Xizhi Dist., New Taipei City 221, Taiwan (R.O.C.)

Test Items		Test Results	Test Methods
Bacterial Filtration	1	99.7	EN 14683:2019 Annex B
Efficiency (BFE)(%)	2	99.8	
Staphylococcus aureus	3	99.7	
ATCC 6538	4	99.7	
	5	99.8	

This test report is for reference only and should not be used as a formal document.

Note: Control average: 2348 CFU.


Note: Mean particle size: 3.0 μ m.

Note: Testing side: outside of specimen.

Note: Testing area: 39.5 cm².

Note: Flow rate : 28.3 L/min.

Note: Sample description is given by the client: ATARAXIS MEDICAL FACE MASK TYPE: II

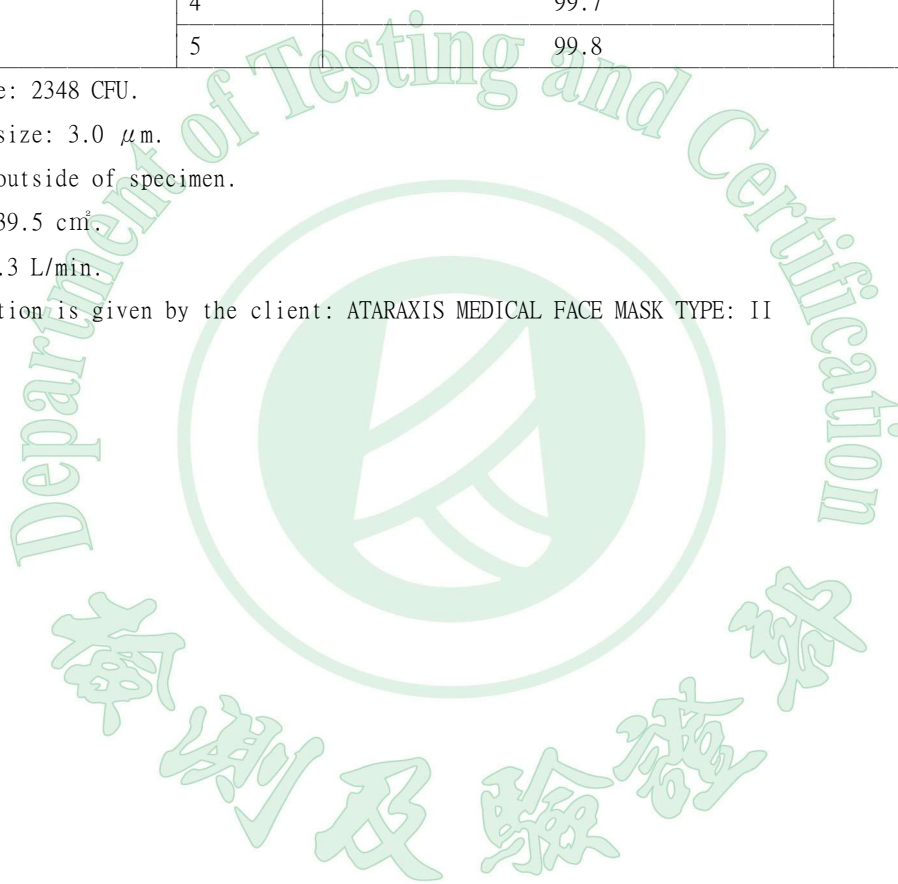

- Note: 1.This report is only responsible for the submitted sample(s), which will be kept for one month period.
- 2.This report cannot be reproduced in any way, except in full context, without the prior approval in writing of this Department of Testing and Certification.
- 3.The test report should not be used for public advertisement and commercial promotion.

Authorized by president of

Taiwan Textile Research Institute

Jui-hung kao

Director,
Department of Testing and
Certification

Department of Testing and Certification, Taiwan Textile Research Institute
No.6, Chengtian Rd., Tucheng Dist., New Taipei City 23674, Taiwan (R.O.C.)
Tel : +886-2-22670321 ext. 7107, 7110
Fax : +886-2-22675108 , +886-2-22689839



TEST REPORT TUCHENG

Date of Issue: Oct.08,2021 Date of Receipt and Test Start: Sep.17,2021

Report No.: TFG01311 Quantity: 1PC Page Order/Pages: (P3/4) Ref. No.: NIL


Report Title: ATARAXIS MEDICAL SUPPLY CO., LTD.(U3494) Item: Mask

Address: 2F., No. 14, Ln. 122, Sec. 2, Xiwan Rd., Xizhi Dist., New Taipei City 221, Taiwan (R.O.C.)

Test Items		Test Results	Test Methods
Microbial cleanliness (cfu/g)	1	10.9	EN 14683:2019
	2	7.6	EN ISO 11737-1:2018
	3	4.2	
	4	1.7	
	5	12.9	

*This test report is for reference only
and should not be used as a formal
document.*

Note: Sample description is given by the client: ATARAXIS MEDICAL FACE MASK TYPE: II

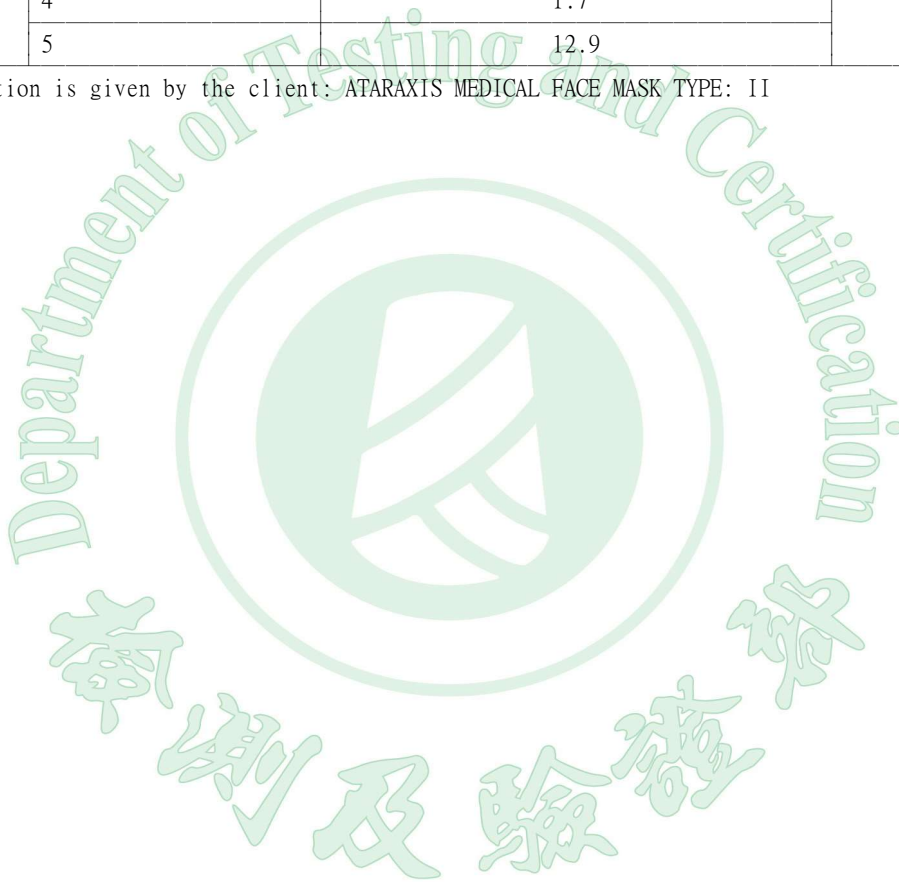

- Note: 1.This report is only responsible for the submitted sample(s), which will be kept for one month period.
- 2.This report cannot be reproduced in any way, except in full context, without the prior approval in writing of this Department of Testing and Certification.
- 3.The test report should not be used for public advertisement and commercial promotion.

Authorized by president of Jui-hung kao
Taiwan Textile Research Institute
Director,
Department of Testing and
Certification

Department of Testing and Certification, Taiwan Textile Research Institute
No.6, Chengtian Rd., Tucheng Dist., New Taipei City 23674, Taiwan (R.O.C.)
Tel : +886-2-22670321 ext. 7107, 7110
Fax : +886-2-22675108 , +886-2-22689839

TEST REPORT TUCHENG

Date of Issue: Oct.08,2021 Date of Receipt and Test Start: Sep.17,2021

Report No.: TFG01311 Quantity: 1PC Page Order/Pages: (P4/4) Ref. No.: NIL

Report Title: ATARAXIS MEDICAL SUPPLY CO., LTD.(U3494) Item: Mask

Address: 2F., No. 14, Ln. 122, Sec. 2, Xiwan Rd., Xizhi Dist., New Taipei City 221, Taiwan (R.O.C.)

*This test report is for reference only
and should not be used as a formal
document.*



TFG01311

- Note: 1.This report is only responsible for the submitted sample(s), which will be kept for one month period.
2.This report cannot be reproduced in any way, except in full context, without the prior approval in writing of this Department of Testing and Certification.
3.The test report should not be used for public advertisement and commercial promotion.

Authorized by president of

Taiwan Textile Research Institute

Jui-hung kao

Director,
Department of Testing and
Certification

Department of Testing and Certification, Taiwan Textile Research Institute
No.6, Chengtian Rd., Tucheng Dist., New Taipei City 23674, Taiwan (R.O.C.)

Tel : +886-2-22670321 ext. 7107, 7110

Fax : +886-2-22675108 , +886-2-22689839